

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00760	Calib. Date: 08/13/2018
Certification File No.:	00761	Calib. No.: 00029
Linearity File No.:	00762	Cert. Date: 08/13/2018
Solution File No.:	00778	Cert. No.: 00024
Sequential File No.:	00778	Lin. Date: 08/13/2018
		Lin. No.: 00023
		Soln. Date: 01/12/2019
		Soln. No.: 00164
		File Date: 01/12/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 1258

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:34S		
Control 1 EC	0.100%	18:35S	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	18:35S	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	18:35S		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature:  #161

Badge No.: 161

Date: 01/12/2019

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0073
Location: BRIELLE POLICE DEPT.
Calibration File No.: 00760 Calib. Date: 08/13/2018 Calib. No.: 00029
Certification File No.: 00761 Cert. Date: 08/13/2018 Cert. No.: 00024
Linearity File No.: 00762 Lin. Date: 08/13/2018 Lin. No.: 00023
Solution File No.: 00779 Soln. Date: 01/12/2019 Soln. No.: 00165
Sequential File No.: 00779 File Date: 01/12/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0052
Control Solution %: 0.100% Expires: 05/10/2020
Solution Control Lot: 18150 Bottle No.: 0964

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:21S		
Control 1 EC	0.099%	21:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:23S		
Control 2 EC	0.099%	21:23S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:24S		
Control 3 EC	0.099%	21:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	21:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:25S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DREHER

First Name: BRIAN

MI: M

Signature: _____

Badge No.: 166

Date: 01/12/2019

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00784	Cert. No.: 00025
Sequential File No.:	00784	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 01/23/2019
		Soln. No.: 00166
		File Date: 01/23/2019

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXA S3-0051
Control Solution %: 0.100%		Expires: 05/10/2020
Solution Control Lot: 18150		Bottle No.: 0972

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:58S		
Control 1 EC	0.101%	10:58S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59S		
Control 2 EC	0.100%	11:00S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:00S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01S		
Control 3 EC	0.100%	11:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDWS P2-227 A

Changed By:

Last Name: PAVLOSKY

First Name: ALLISON

MI: M.

Signature:  7330

Badge No.: 7330

Date: 01/23/2019

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00787	Cert. No.: 00025
Sequential File No.:	00787	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 02/18/2019
		Soln. No.: 00167
		File Date: 02/18/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 1031

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:42S		
Control 1 EC	0.099%	09:42S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:42S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		
Control 2 EC	0.097%	09:44S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45S		
Control 3 EC	0.098%	09:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Sgt. R. SOFIELD #161

Badge No.: 161

Date: 02/18/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00789	Cert. No.: 00025
Sequential File No.:	00789	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 03/15/2019
		Soln. No.: 00168
		File Date: 03/15/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 1086

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:19S		
Control 1 EC	0.099%	05:20S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:21S		
Control 2 EC	0.097%	05:21S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:22S		
Control 3 EC	0.099%	05:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:24S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Sgt. [Signature] #161

Badge No.: 161

Date: 03/15/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00796	Cert. No.: 00025
Sequential File No.:	00796	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 05/05/2019
		Soln. No.: 00170
		File Date: 05/05/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 0973

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:39D		
Control 1 EC	0.101%	14:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:40D		
Control 2 EC	0.099%	14:41D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:42D		
Control 3 EC	0.100%	14:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CUSACK

First Name: BRANDON

MI: A

Signature: *PH. Brandon Cusack #168*

Badge No.: 168

Date: 05/05/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00800	Cert. No.: 00025
Sequential File No.:	00800	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 05/28/2019
		Soln. No.: 00171
		File Date: 05/28/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 0917

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:02D		
Control 1 EC	0.100%	13:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:03D		
Control 2 EC	0.099%	13:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	13:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:05D		
Control 3 EC	0.100%	13:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____



Badge No.: 161

Date: 05/28/2019

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00781	Calib. Date: 01/23/2019
Certification File No.:	00782	Calib. No.: 00030
Linearity File No.:	00783	Cert. Date: 01/23/2019
Solution File No.:	00806	Cert. No.: 00025
Sequential File No.:	00806	Lin. Date: 01/23/2019
		Lin. No.: 00024
		Soln. Date: 06/22/2019
		Soln. No.: 00173
		File Date: 06/22/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 1143

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:15D		
Control 1 EC	0.100%	22:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	22:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:16D		
Control 2 EC	0.099%	22:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	22:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:17D		
Control 3 EC	0.099%	22:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Sgt. [Signature] #161

Badge No.: 161

Date: 06/22/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00807	Calib. Date:	06/24/2019
Certification File No.:	00808	Cert. No.:	00031
Linearity File No.:	00809	Lin. Date:	06/24/2019
Solution File No.:	00810	Cert. No.:	00026
Sequential File No.:	00810	Lin. No.:	00025
		Soln. Date:	06/24/2019
		Soln. No.:	00174
		File Date:	06/24/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0052
Solution Control Lot:	19060	Expires:	02/11/2021
		Bottle No.:	0186

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:59D		
Control 1 EC	0.101%	14:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		
Control 2 EC	0.100%	15:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:01D		
Control 3 EC	0.101%	15:02D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDWJP2-228 (D)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

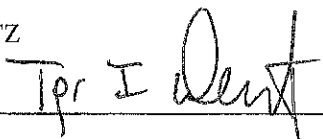Signature: 

7045

Badge No.: 7045

Date: 06/24/2019

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00807	Calib. Date: 06/24/2019
Certification File No.:	00808	Calib. No.: 00031
Linearity File No.:	00809	Cert. Date: 06/24/2019
Solution File No.:	00815	Cert. No.: 00026
Sequential File No.:	00815	Lin. Date: 06/24/2019
		Lin. No.: 00025
		Soln. Date: 07/17/2019
		Soln. No.: 00175
		File Date: 07/17/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0127

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:04D		
Control 1 EC	0.099%	16:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:05D		
Control 2 EC	0.098%	16:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:06D		
Control 3 EC	0.098%	16:07D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Badge No.: 161

Date: 07/17/2019

Calibrating Unit

New Standard Solution Report


Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00807	Calib. Date:	06/24/2019
Certification File No.:	00808	Cert. No.:	00031
Linearity File No.:	00809	Cert. Date:	06/24/2019
Solution File No.:	00818	Lin. No.:	00025
Sequential File No.:	00818	Lin. Date:	06/24/2019
		Soln. Date:	08/10/2019
		Soln. No.:	00176
		File Date:	08/10/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0052
Solution Control Lot:	19060	Expires:	02/11/2021
		Bottle No.:	0126

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:41D		
Control 1 EC	0.100%	18:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:42D		
Control 2 EC	0.099%	18:43D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:43D		
Control 3 EC	0.099%	18:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD	First Name: RONALD	MI: G
Signature: 	Badge No.: 161	Date: 08/10/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00807	Calib. Date: 06/24/2019
Certification File No.:	00808	Calib. No.: 00031
Linearity File No.:	00809	Cert. Date: 06/24/2019
Solution File No.:	00825	Cert. No.: 00026
Sequential File No.:	00825	Lin. Date: 06/24/2019
		Lin. No.: 00025
		Soln. Date: 09/04/2019
		Soln. No.: 00177
		File Date: 09/04/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0124

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:24D		
Control 1 EC	0.100%	05:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:25D		
Control 2 EC	0.099%	05:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:26D		
Control 3 EC	0.099%	05:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:27D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Badge No.: 161

Date: 09/04/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00807	Calib. Date: 06/24/2019
Certification File No.:	00808	Calib. No.: 00031
Linearity File No.:	00809	Cert. Date: 06/24/2019
Solution File No.:	00832	Cert. No.: 00026
Sequential File No.:	00832	Lin. Date: 06/24/2019
		Lin. No.: 00025
		Soln. Date: 09/26/2019
		Soln. No.: 00178
		File Date: 09/26/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0197

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:52D		
Control 1 EC	0.098%	17:53D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	17:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:54D		
Control 2 EC	0.098%	17:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:55D		
Control 3 EC	0.099%	17:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Badge No.: 161

Date: 09/26/2019

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0073
Location: BRIELLE POLICE DEPT.
Calibration File No.: 00807 Calib. Date: 06/24/2019 Calib. No.: 00031
Certification File No.: 00808 Cert. Date: 06/24/2019 Cert. No.: 00026
Linearity File No.: 00809 Lin. Date: 06/24/2019 Lin. No.: 00025
Solution File No.: 00833 Soln. Date: 10/25/2019 Soln. No.: 00179
Sequential File No.: 00833 File Date: 10/25/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0052
Control Solution %: 0.100% Expires: 02/11/2021
Solution Control Lot: 19060 Bottle No.: 0199

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:30D		
Control 1 EC	0.101%	05:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:31D		
Control 2 EC	0.099%	05:31D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	05:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:32D		
Control 3 EC	0.099%	05:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	05:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:33D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____



Badge No.: 161

Date: 10/25/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00807	Calib. Date: 06/24/2019
Certification File No.:	00808	Calib. No.: 00031
Linearity File No.:	00809	Cert. Date: 06/24/2019
Solution File No.:	00834	Cert. No.: 00026
Sequential File No.:	00834	Lin. Date: 06/24/2019
		Lin. No.: 00025
		Soln. Date: 11/17/2019
		Soln. No.: 00180
		File Date: 11/17/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0132

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:14S		
Control 1 EC	0.102%	16:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:15S		
Control 2 EC	0.100%	16:16S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:17S		
Control 3 EC	0.100%	16:17S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:18S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____

Sgt. [Signature] #161

Badge No.: 161

Date: 11/17/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00836	Calib. Date:	12/05/2019
Certification File No.:	00837	Cert. No.:	00032
Linearity File No.:	00838	Lin. Date:	12/05/2019
Solution File No.:	00839	Cert. No.:	00027
Sequential File No.:	00839	Lin. No.:	00026
		Soln. Date:	12/05/2019
		Soln. No.:	00181
		File Date:	12/05/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0051
Solution Control Lot:	19060	Expires:	02/11/2021
		Bottle No.:	0410

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:15S		
Control 1 EC	0.101%	14:15S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:16S		
Control 2 EC	0.099%	14:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:18S		
Control 3 EC	0.100%	14:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:19S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDWJPL-227 (DL)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

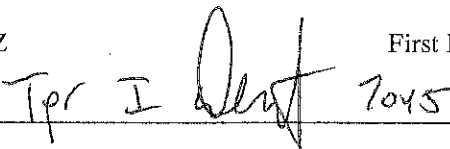Signature: 

Badge No.: 7045

Date: 12/05/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00836	Calib. Date: 12/05/2019
Certification File No.:	00837	Calib. No.: 00032
Linearity File No.:	00838	Cert. Date: 12/05/2019
Solution File No.:	00842	Cert. No.: 00027
Sequential File No.:	00842	Lin. Date: 12/05/2019
		Lin. No.: 00026
		Soln. Date: 12/29/2019
		Soln. No.: 00182
		File Date: 12/29/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0139

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:22S		
Control 1 EC	0.099%	19:23S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:23S		
Control 2 EC	0.097%	19:24S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	19:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:25S		
Control 3 EC	0.097%	19:26S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:26S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:26S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: _____



Badge No.: 161

Date: 12/29/2019