

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00836	Calib. Date:	12/05/2019
Certification File No.:	00837	Cert. No.:	00032
Linearity File No.:	00838	Cert. Date:	12/05/2019
Solution File No.:	00843	Lin. No.:	00026
Sequential File No.:	00843	Lin. Date:	12/05/2019
		Soln. Date:	01/23/2020
		Soln. No.:	00183
		File Date:	01/23/2020

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0051
Control Solution %:	0.100%			Expires:	02/11/2021
Solution Control Lot:	19060			Bottle No.:	0136

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:33S		
Control 1 EC	0.099%	14:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:35S		
Control 2 EC	0.097%	14:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:36S		
Control 3 EC	0.098%	14:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_



Badge No.: 161

Date: 01/23/2020

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00836	Calib. Date: 12/05/2019
Certification File No.:	00837	Calib. No.: 00032
Linearity File No.:	00838	Cert. Date: 12/05/2019
Solution File No.:	00847	Cert. No.: 00027
Sequential File No.:	00847	Lin. Date: 12/05/2019
		Lin. No.: 00026
		Soln. Date: 02/07/2020
		Soln. No.: 00184
		File Date: 02/07/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	19060	Expires: 02/11/2021
		Bottle No.: 0191

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:09S		
Control 1 EC	0.096%	20:09S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:10S		
Control 2 EC	0.096%	20:11S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	20:11S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:11S		
Control 3 EC	0.097%	20:12S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:12S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:13S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_



Badge No.: 161

Date: 02/07/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00836	Calib. Date:	12/05/2019
Certification File No.:	00837	Cert. No.:	00032
Linearity File No.:	00838	Lin. Date:	12/05/2019
Solution File No.:	00848	Cert. No.:	00027
Sequential File No.:	00848	Lin. No.:	00026
		Soln. Date:	03/06/2020
		Soln. No.:	00185
		File Date:	03/06/2020

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXA S3-0051
Control Solution %:	0.100%			Expires:	02/11/2021
Solution Control Lot:	19060			Bottle No.:	0194

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:52S		
Control 1 EC	0.100%	07:52S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	07:52S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:53S		
Control 2 EC	0.097%	07:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:55S		
Control 3 EC	0.099%	07:55S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_



Badge No.: 161

Date: 03/06/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00836	Calib. Date: 12/05/2019
Certification File No.:	00837	Calib. No.: 00032
Linearity File No.:	00838	Cert. Date: 12/05/2019
Solution File No.:	00850	Cert. No.: 00027
Sequential File No.:	00850	Lin. Date: 12/05/2019
		Lin. No.: 00026
		Soln. Date: 04/03/2020
		Soln. No.: 00186
		File Date: 04/03/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1353

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:41S		
Control 1 EC	0.097%	18:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	18:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:42S		
Control 2 EC	0.096%	18:43S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:44S		
Control 3 EC	0.096%	18:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	18:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:45S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

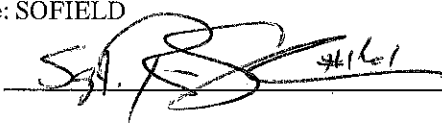

Badge No.: 161

Date: 04/03/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00836	Calib. Date: 12/05/2019
Certification File No.:	00837	Calib. No.: 00032
Linearity File No.:	00838	Cert. Date: 12/05/2019
Solution File No.:	00851	Cert. No.: 00027
Sequential File No.:	00851	Lin. Date: 12/05/2019
		Lin. No.: 00026
		Soln. Date: 04/28/2020
		Soln. No.: 00187
		File Date: 04/28/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1305

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:49D		
Control 1 EC	0.098%	08:49D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:49D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50D		
Control 2 EC	0.096%	08:51D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:52D		
Control 3 EC	0.097%	08:52D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

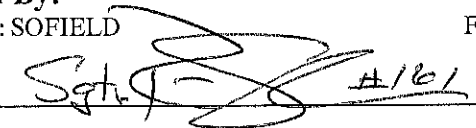

Badge No.: 161

Date: 04/28/2020

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARWM-0073
Location:	BRIELLE POLICE DEPT.		
Calibration File No.:	00852	Calib. Date:	05/18/2020
Certification File No.:	00853	Cert. No.:	00033
Linearity File No.:	00854	Cert. Date:	05/18/2020
Solution File No.:	00856	Lin. No.:	00027
Sequential File No.:	00856	Soln. Date:	06/12/2020
		Soln. No.:	00189
		File Date:	06/12/2020
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXA S3-0052
Solution Control Lot:	19300	Expires:	10/30/2021
		Bottle No.:	1288

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:09D		
Control 1 EC	0.100%	09:10D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		
Control 2 EC	0.099%	09:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:12D		
Control 3 EC	0.099%	09:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

*Sgt. [Signature]* #161

Badge No.: 161

Date: 06/12/2020

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00852	Calib. Date: 05/18/2020
Certification File No.:	00853	Calib. No.: 00033
Linearity File No.:	00854	Cert. Date: 05/18/2020
Solution File No.:	00859	Cert. No.: 00028
Sequential File No.:	00859	Lin. Date: 05/18/2020
		Lin. No.: 00027
		Soln. Date: 06/23/2020
		Soln. No.: 00190
		File Date: 06/23/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1292

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:40D		
Control 1 EC	0.097%	08:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	08:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:41D		
Control 2 EC	0.096%	08:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	08:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:43D		
Control 3 EC	0.096%	08:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

Badge No.: 161

Date: 06/23/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00852	Calib. Date: 05/18/2020
Certification File No.:	00853	Calib. No.: 00033
Linearity File No.:	00854	Cert. Date: 05/18/2020
Solution File No.:	00861	Cert. No.: 00028
Sequential File No.:	00861	Lin. Date: 05/18/2020
		Lin. No.: 00027
		Soln. Date: 07/17/2020
		Soln. No.: 00191
		File Date: 07/17/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1304

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:50D		
Control 1 EC	0.100%	04:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:52D		
Control 2 EC	0.098%	04:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:53D		
Control 3 EC	0.098%	04:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_



Badge No.: 161

Date: 07/17/2020



# Calibrating Unit

## New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00852	Calib. Date: 05/18/2020
Certification File No.:	00853	Calib. No.: 00033
Linearity File No.:	00854	Cert. Date: 05/18/2020
Solution File No.:	00863	Cert. No.: 00028
Sequential File No.:	00863	Lin. Date: 05/18/2020
		Lin. No.: 00027
		Soln. Date: 08/10/2020
		Soln. No.: 00192
		File Date: 08/10/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0052
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1326

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:14D		
Control 1 EC	0.100%	05:14D	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	05:14D	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	05:15D		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD	First Name: RONALD	MI: G
Signature:  #161	Badge No.: 161	Date: 08/10/2020

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWM-0073  
Location: BRIELLE POLICE DEPT.  
Calibration File No.: 00852 Calib. Date: 05/18/2020 Calib. No.: 00033  
Certification File No.: 00853 Cert. Date: 05/18/2020 Cert. No.: 00028  
Linearity File No.: 00854 Lin. Date: 05/18/2020 Lin. No.: 00027  
Solution File No.: 00864 Soln. Date: 08/10/2020 Soln. No.: 00193  
Sequential File No.: 00864 File Date: 08/10/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0052  
Control Solution %: 0.100% Expires: 10/31/2021  
Solution Control Lot: 19300 Bottle No.: 1290

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:32D		
Control 1 EC	0.099%	06:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	06:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:33D		
Control 2 EC	0.098%	06:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:35D		
Control 3 EC	0.099%	06:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	06:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


## Changed By:

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

 #161

Badge No.: 161

Date: 08/10/2020

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARWM-0073  
Location: BRIELLE POLICE DEPT.  
Calibration File No.: 00869 Calib. Date: 09/01/2020 Calib. No.: 00034  
Certification File No.: 00870 Cert. Date: 09/01/2020 Cert. No.: 00029  
Linearity File No.: 00871 Lin. Date: 09/01/2020 Lin. No.: 00028  
Solution File No.: 00872 Soln. Date: 09/01/2020 Soln. No.: 00196  
Sequential File No.: 00872 File Date: 09/01/2020

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0051  
Control Solution %: 0.100% Expires: 10/30/2021  
Solution Control Lot: 19300 Bottle No.: 1296

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:16D		
Control 1 EC	0.101%	10:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:17D		
Control 2 EC	0.100%	10:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18D		
Control 3 EC	0.100%	10:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJP2-227 DL

### Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpr I Dent 7045

Badge No.: 7045

Date: 09/01/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00869	Calib. Date: 09/01/2020
Certification File No.:	00870	Calib. No.: 00034
Linearity File No.:	00871	Cert. Date: 09/01/2020
Solution File No.:	00874	Lin. Date: 09/01/2020
Sequential File No.:	00874	Soln. Date: 09/26/2020
		Soln. No.: 00197
		File Date: 09/26/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	19300	Expires: 10/30/2021
		Bottle No.: 1315

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:29D		
Control 1 EC	0.098%	12:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 2 EC	0.098%	12:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	12:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:31D		
Control 3 EC	0.098%	12:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

Sgt. [Signature] #161

Badge No.: 161

Date: 09/26/2020

# Calibrating Unit

## New Standard Solution Report


<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00869	Calib. Date: 09/01/2020
Certification File No.:	00870	Calib. No.: 00034
Linearity File No.:	00871	Cert. Date: 09/01/2020
Solution File No.:	00875	Cert. No.: 00029
Sequential File No.:	00875	Lin. Date: 09/01/2020
		Lin. No.: 00028
		Soln. Date: 10/21/2020
		Soln. No.: 00198
		File Date: 10/21/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	20390	Expires: 09/02/2022
		Bottle No.: 1146

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:16D		
Control 1 EC	0.098%	11:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17D		
Control 2 EC	0.099%	11:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18D		
Control 3 EC	0.098%	11:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD	First Name: RONALD	MI: G
Signature: <u></u>	Badge No.: 161	Date: 10/21/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00869	Calib. Date: 09/01/2020
Certification File No.:	00870	Calib. No.: 00034
Linearity File No.:	00871	Cert. Date: 09/01/2020
Solution File No.:	00880	Cert. No.: 00029
Sequential File No.:	00880	Lin. Date: 09/01/2020
		Lin. No.: 00028
		Soln. Date: 11/16/2020
		Soln. No.: 00199
		File Date: 11/16/2020

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDXA S3-0051
Control Solution %: 0.100%		Expires: 09/02/2022
Solution Control Lot: 20390		Bottle No.: 0061

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:10S		
Control 1 EC	0.099%	06:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:12S		
Control 2 EC	0.098%	06:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	06:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13S		
Control 3 EC	0.098%	06:14S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature:  #161

Badge No.: 161

Date: 11/16/2020

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0073
Location:	BRIELLE POLICE DEPT.	
Calibration File No.:	00869	Calib. Date: 09/01/2020
Certification File No.:	00870	Calib. No.: 00034
Linearity File No.:	00871	Cert. Date: 09/01/2020
Solution File No.:	00882	Cert. No.: 00029
Sequential File No.:	00882	Lin. Date: 09/01/2020
		Lin. No.: 00028
		Soln. Date: 12/11/2020
		Soln. No.: 00200
		File Date: 12/11/2020
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0051
Solution Control Lot:	20390	Expires: 09/02/2022
		Bottle No.: 1049

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:25S		
Control 1 EC	0.097%	09:25S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26S		
Control 2 EC	0.097%	09:27S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.096%	09:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:27S		
Control 3 EC	0.096%	09:28S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:29S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SOFIELD

First Name: RONALD

MI: G

Signature: \_\_\_\_\_

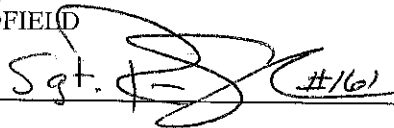

Badge No.: 161

Date: 12/11/2020