

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMH-0287  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 07/06/2022  
Time: 08:08:55

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
**Brielle Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0287  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 38 Wet Adjust Date: 07/06/2022 Wet Adjust No.: 1  
Wet Adjust Time: 09:39:19

Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARND-0001 Adj. Unit Exp.: 01/13/2023  
Solution Lot No.: 21210 Soln. Bottle No.: 265 Adjust Soln. Exp.: 06/16/2023

Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.00 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*Sgt. K A 6704*

Signed:

Date: 07/06/2022

ID: 1

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
**Brielle Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0287  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 39 Dry Adjust Date: 07/06/2022 Dry Adjust No.: 1  
Dry Adjust Time: 10:01:27

Concentration: 0.100 %  
Dry Gas Lot No.: 1460885 Adjust Gas Exp.: 03/12/2024  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001270 Barom. Cert. Exp.: 12/01/2022  
Pre-adjust Amb. Pressure: 1010 hPa Post-adjust Amb. Pressure: 1009 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*Sgt /K 2 6704*

Signed:

Date: 07/06/2022

ID: 1

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
**Brielle Borough**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0287  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 40 Lin. Date: 07/06/2022 Lin. No.: 1

0.040% Dry Gas Lot No.: 1486624 Adjust. Gas Exp.: 04/26/2024  
0.080% Dry Gas Lot No.: 1346773 Adjust. Gas Exp.: 07/08/2023  
0.160% Dry Gas Lot No.: 1523726 Adjust. Gas Exp.: 07/16/2024  
0.300% Dry Gas Lot No.: 1495468 Adjust. Gas Exp.: 05/14/2024

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	10:06:56		*TEST PASSED*
Control .04 Test 1 EC	0.039	10:07:34	1009	*TEST PASSED*
Control .04 Test 1 IR	0.038	10:07:34	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:08:27		*TEST PASSED*
Control .04 Test 2 EC	0.040	10:08:41	1009	*TEST PASSED*
Control .04 Test 2 IR	0.039	10:08:41	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:10:17		*TEST PASSED*
Control .08 Test 3 EC	0.079	10:10:53	1009	*TEST PASSED*
Control .08 Test 3 IR	0.079	10:10:53	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:11:51		*TEST PASSED*
Control .08 Test 4 EC	0.081	10:12:06	1009	*TEST PASSED*
Control .08 Test 4 IR	0.080	10:12:06	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:13:34		*TEST PASSED*
Control .16 Test 5 EC	0.159	10:14:11	1009	*TEST PASSED*
Control .16 Test 5 IR	0.160	10:14:11	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:15:15		*TEST PASSED*
Control .16 Test 6 EC	0.161	10:15:30	1009	*TEST PASSED*
Control .16 Test 6 IR	0.162	10:15:30	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:16:55		*TEST PASSED*
Control .30 Test 7 EC	0.301	10:17:31	1009	*TEST PASSED*
Control .30 Test 7 IR	0.303	10:17:31	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:18:42		*TEST PASSED*
Control .30 Test 8 EC	0.307	10:18:57	1009	*TEST PASSED*
Control .30 Test 8 IR	0.306	10:18:57	1009	*TEST PASSED*
Ambient Air Blank	0.000	10:19:18		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*Sgt AK A 6704*

Signed:

Date: 07/06/2022

ID: 1

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
**Brielle Borough**  
**SERIAL NUMBER: ARMH-0287**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0287  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl1 Install File No.: 41 Cyl1 Install Date: 07/06/2022 Cyl1 Install No.: 1

**Control Tests (0.100%)**

Installation Inlet: #1 (Upper) Post test active Cyl.: #1 (Upper)  
 Dry Gas Lot No.: 302-402396000 Dry Gas Lot Exp.: 03/21/2025

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	10:31:03		*TEST PASSED*
Control Test 1			1009	*TEST PASSED*
EC Result	0.100	10:31:50		*TEST PASSED*
IR Result	0.100	10:31:50		*TEST PASSED*
Ambient Air Blank	0.000	10:32:51		*TEST PASSED*
Control Test 2			1009	*TEST PASSED*
EC Result	0.101	10:33:15		*TEST PASSED*
IR Result	0.101	10:33:15		*TEST PASSED*
Ambient Air Blank	0.000	10:34:16		*TEST PASSED*
Control Test 3			1009	*TEST PASSED*
EC Result	0.101	10:34:40		*TEST PASSED*
IR Result	0.101	10:34:40		*TEST PASSED*
Ambient Air Blank	0.000	10:35:01		*TEST PASSED*

**Result**

**All tests within acceptable tolerance.**

**Coordinator**

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*SKG 6704*

Signed:

Date: 07/06/2022

ID: 1

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
**Brielle Borough**  
**SERIAL NUMBER: ARMH-0287**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMH-0287  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
Cyl2 Install File No.: 42 Cyl2 Install Date: 07/06/2022 Cyl2 Install No.: 1

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
Dry Gas Lot No.: 302-402410761 Dry Gas Lot Exp.: 04/14/2025

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	11:06:35		*TEST PASSED*
Control Test 1			1009	*TEST PASSED*
EC Result	0.101	11:07:21		*TEST PASSED*
IR Result	0.102	11:07:21		*TEST PASSED*
Ambient Air Blank	0.000	11:08:21		*TEST PASSED*
Control Test 2			1009	*TEST PASSED*
EC Result	0.102	11:08:45		*TEST PASSED*
IR Result	0.102	11:08:45		*TEST PASSED*
Ambient Air Blank	0.000	11:09:47		*TEST PASSED*
Control Test 3			1009	*TEST PASSED*
EC Result	0.102	11:10:11		*TEST PASSED*
IR Result	0.102	11:10:11		*TEST PASSED*
Ambient Air Blank	0.000	11:10:32		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: ALCOTT - First Name: KEVIN MI: W Badge No.: 6704

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*Sgt K G 6704*

Signed:

Date: 07/06/2022

ID: 1



# State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

PHILIP D. MURPHY  
*Governor*

SHEILA Y. OLIVER  
*Lt. Governor*

GURBIR S. GREWAL  
*Attorney General*

PATRICK J. CALAHAN  
*Colonel*

## CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Dräger, Inc.

**ANALYSIS DATE:** 07/07/2021

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 21210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1199 to 0.1215 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 16, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Michael Kennedy*  
Michael Kennedy  
Assistant Chief Forensic Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of July, 2021.

*[Signature]*  
Notary

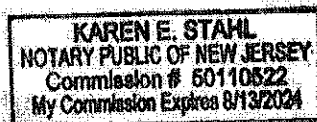

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable



**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S104302598632



## Certificate/SO Number: 5-D6Z1H-60-1 Revision 0

**Manufacturer:** Dräger Safety AG & Co. KGaA  
**Model Number:** X-Cal 2000  
**Description:** Breath Alcohol Simulator  
**Serial Number:** ARND-0001  
**ID:** NONE

**As-Found:** In Tolerance  
**As-Left:** In Tolerance  
**Issue Date:** Jan 13, 2022  
**Calibration Date:** Jan 13, 2022  
**Due Date:** Jan 13, 2023

**Calibrated To:** Customer Specification  
**Calibration Procedure:** 1-AC103519-1

Transcat Calibration Laboratories have been audited and found in compliance with ISO /IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual OAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/NCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANSI/NCSL Z540.3:2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations: Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).





Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104302598632

**Certificate/SO Number: 5-D6Z1H-60-1 Revision 0**

**As Found/As Left Data**

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	O T	Cal Process Uncertainty (k=2; #)	Measurement Uncertainty (k=2; #)	Units	TUR
<b>Function Checks</b>										
Bubble Check			P	P	P					
Seal Check			P	P	P					
<b>Temperature Source: Accuracy Test</b>										
Accuracy Test	34.00°C	±(0.02 °C)	33.98	34.02	34.01 °C		1.1e-002	1.6e-002	°C	1.8 : 1
<b>Temperature Source: Stability Test</b>										
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C		1.1e-002	1.6e-002	°C	1.8 : 1

Field not applicable.

**Traceable Standards**

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
05H1277	AccuMac Corporation	AM1760-12-S	Secondary SPRT	27-May-21	31-May-22	15-80SH1277-3-1	AF/AL
FP927312	Hart Scientific/Fluke	1575	Super Thermometer	18-May-21	30-Nov-22	5-8HP927312-5-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.


**Environmental Data**

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
70.52°F / 21.40°C	36.80%	DewK6	G	Temperature

**Decision Rule**

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows : The acceptance zone is defined as: less than or equal

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S1O4302598632

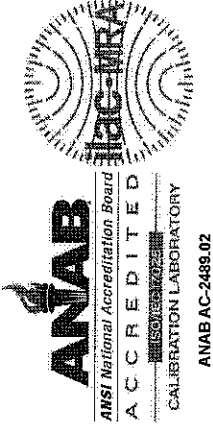

**Certificate/SO Number: 5-D6Z1H-60-1 Revision 0**

to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S104302598632




**Certificate/SO Number: 5-D6Z1H-60-1 Revision 0**

**Legend**

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

**Customer:** DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
**PO Number:** S1O4302598632

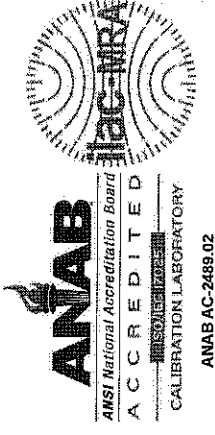

**Certificate/SO Number:** 5-D6Z1H-60-1 Revision 0

**Calibrated At:**  
16115 Park Row  
Houston, TX 77084

**Facility Responsible:**  
16115 Park Row  
Houston, TX 77084  
800-828-1470

**Unit Barcode:** 0900B4365  
0900B43653

**Date Received:** January 12, 2022  
**Service Level:** R9

**Calibrated By:**  
  
Camden Alford

**Electronically Signed By:**  
Camden Alford  
Jan 13, 2022  
12:41:00 -05:00

**Reviewed By:**  
  
Josh Solleau for

**Electronically Signed By:**  
Scott D. Caine  
Lab Manager  
Jan 13, 2022  
14:06:08 -05:00

**Certificate - Page 5 of 5**  
Reprinted on January 19, 2022

**Customer Number:** 1-659111-000  
OPS-F20-014R10 09/29/21 F P001R9 4/9/2021

# CALIBRATED BY TRANSCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC

7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104302546636

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

Manufacturer: Wika Instr/Mensor Corp/Trend  
Model Number: CPG2300

Description: Portable Barometer  
Serial Number: 41001270  
ID: NONE

As-Found: In Tolerance  
As-Left: In Tolerance  
Issue Date: Dec 01, 2021  
Calibration Date: Dec 01, 2021  
Due Date: Dec 01, 2022

Calibrated To: Manufacturer Specification  
Calibration Procedure: 1-AC107288-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-008, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/MCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS16949:2009, 10CFR21, 10CFR50 App. B, ASME NQA-1:2012, and ANS/MCSL Z540.2-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate. Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.


Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International R19-18. For mass calibrations: Conventional mass (referenced to 8.0 g/cm<sup>3</sup>).

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturer's (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a shift in tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).



# CALIBRATED BY TMS&S CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77095  
 PO Number: S104302546536

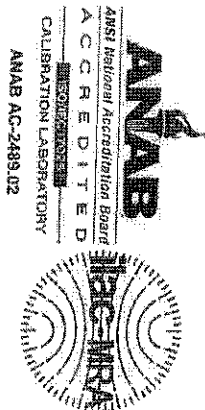

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

As Found/As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found / As Left	Cal Process Uncertainty (k=2; z)	Measurement Uncertainty (k=2; z)	Units	TUR
Pressure Measure: 562 to 1172 mbara Range									
	550.1 mbara	±(0.015% FS)	549.9	550.3	550.1 mbara	1.0e-002	1.2e-001	mbara	19.1 : 1
	610.0 mbara	±(0.015% FS)	609.8	610.2	610.0 mbara	1.2e-002	1.2e-001	mbara	17.3 : 1
	680.4 mbara	±(0.015% FS)	680.2	680.6	680.4 mbara	1.3e-002	1.2e-001	mbara	15.5 : 1
	734.3 mbara	±(0.015% FS)	734.1	734.5	734.3 mbara	1.4e-002	1.2e-001	mbara	14.3 : 1
	804.7 mbara	±(0.015% FS)	804.5	804.9	804.6 mbara	1.5e-002	1.2e-001	mbara	13.1 : 1
	864.9 mbara	±(0.015% FS)	864.7	865.1	864.9 mbara	1.6e-002	1.2e-001	mbara	12.2 : 1
	924.9 mbara	±(0.015% FS)	924.7	925.1	924.9 mbara	1.8e-002	1.2e-001	mbara	11.4 : 1
	985.2 mbara	±(0.015% FS)	985.0	985.4	985.2 mbara	1.9e-002	1.2e-001	mbara	10.7 : 1
	1043.9 mbara	±(0.015% FS)	1043.7	1044.1	1043.9 mbara	2.0e-002	1.3e-001	mbara	10.1 : 1
	1114.2 mbara	±(0.015% FS)	1114.0	1114.4	1114.2 mbara	2.1e-002	1.2e-001	mbara	9.4 : 1
	1174.6 mbara	±(0.015% FS)	1174.4	1174.8	1174.6 mbara	2.2e-002	1.2e-001	mbara	9.0 : 1
	924.9 mbara	±(0.015% FS)	924.7	925.1	924.9 mbara	1.8e-002	1.2e-001	mbara	11.4 : 1
	864.9 mbara	±(0.015% FS)	864.7	865.1	864.9 mbara	1.6e-002	1.2e-001	mbara	12.2 : 1
	804.7 mbara	±(0.015% FS)	804.5	804.9	804.6 mbara	1.5e-002	1.2e-001	mbara	13.1 : 1


Field not applicable.

Date Received: November 15, 2021  
 Service Level: R9

# CALIBRATED BY TRASCAT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104302546536

Certificate/SO Number: 5-GG5JD-40-1 Revision 0

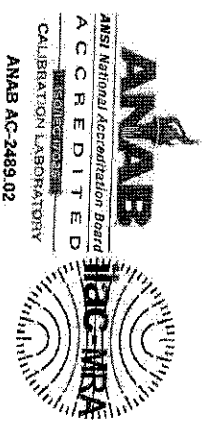

### Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW11BA	Fuke/DH Instruments	PG7601	Piston Gauge	5-Apr-21	5-Apr-22	5-8DW11BA-10-1	AF/AL
DW11CA	Fuke/DH Instruments	MS-AMH-38	AMH Mass Set	3-Sep-21	3-Dec-21	5-8DW11CA-10-1	AF/AL
DW11LOW	Fuke/DH Instruments	PC-71007/800-10-TC	Gas Piston-Cylinder Module	2-Mar-17	31-Mar-22	5-8DW11LOW-1-1	AF/AL
DW11MASS	Fuke/DH Instruments	MS-AMH-38	AMH Mass Set	4-Jun-20	31-Dec-21	5-8DW11MASS-4-1	AF/AL

The use of the standard is defined as: Af - used for as-found readings, AL - used for as-left readings.

### Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
71.57°F /21.98°C	47.20%	DewK5	B	Secondary Pressure

### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results in the acceptance zone measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone for repeated identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance(OOT) and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

# CALIBRATED BY TRACEKIT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: S104302546536

Certificate/SO Number: 5-GG5JD-40-1 Revision 0



Topic	Description	Legend
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances	
As Found	Initial measurement results	
As Left	Measurement results after adjustment and/or repair	
Blank Data Field	Test is not applicable for the UUT	
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result	
Calibration Date	Indicates the date that the calibration was completed	
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result	
Due Date	Indicates the end of the calibration cycle as requested by the customer	
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued	
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement	
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity	
OOA	Out of Acceptance (#)	
OOT	Out of Tolerance (*)	
Setpoints	Measurement target values	
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)	
Traceability Number	Unique Identifier(s) used to document traceability of calibration standards	
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results	
UUT	Unit Under test	


Date Received: November 15, 2021  
 Service Level: R9



# CALIBRATED BY TRANSCIT CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: S104302546536

Certificate/SO Number: 5-GG5UD-40-1 Revision 0

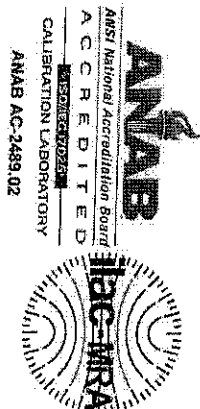

Calibrated At:  
16115 Park Row  
Houston, TX 77084

Facility Responsible:  
16115 Park Row  
Houston, TX 77084  
800-828-1470

Unit Barcode:



0900B429641

Date Received: November 15, 2021  
Service Level: R9

Calibrated By:

Electronically Signed By:  
Fritz Cardona

Fritz Cardona  
Calibration Technician  
Dec 01, 2021  
09:27:49 -05:00

Reviewed By:

Electronically Signed By:  
Scott D. Caine

Scott D. Caine  
Lab Manager  
Dec 01, 2021  
09:49:04 -05:00



**CERTIFICATE OF ANALYSIS**  
**EBS - ETHANOL BREATH STANDARD**

DRAEGER, INC  
1221 S. BELTLINE RD, STE 700  
COPPELL TX 75019

INVOICE#: 20908188  
PO#: US44302331960  
CUST. ITEM #: 4401036  
DATE: Mar. 19, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 1460885  
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Mar. 12, 2024

COMPONENT	PPM	( BrAC )
ETHANOL	260.5	(0.100)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	262.8	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

\* CERTIFICATION TRACEABLE TO National Metrology Institute Traceable Standards.

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.  
Calibration test 121088, 121097, 121091, or 121100 dated, 18th January 2019 applies.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.  
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Mar. 12, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY :

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410)228-6400 Fax: (410)228-4251

# ANALYSIS CERTIFICATION

METHOD OF PREPARATION : GRAVIMETRIC / PRESSURE TRANSFILLING

METHOD OF ANALYSIS : IR Breath Alcohol Analyzer

ACCURACY :  $\pm 0.002$  BrAC or  $\pm 2\%$  whichever is greater.

LOT NO. & QTY.	COMP. 1 C <sub>2</sub> H <sub>5</sub> OH	COMP. 2 N <sub>2</sub>	COMP. 3	COMP. 4	COMP. 5	COMP. 6	Exp Date
1486624 (8)	104.2PPM (0.040 BrAC)	BALANCE					04/26/24

## TRACEABILITY

Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited Company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

WEIGHT SETS USED: Kit#80141, Test#3094344A, Kit#106, 27, 103, 107, 113, 22, Test#VA-21-12587-L,F,T,P, Kit#IM1966, Test#VA-21-12587N, Kit#35, 104, 39, 105, 108, 109, 111 Test#VA-21-12587-I.

No affecting environmental conditions during analysis.

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

REQUESTED BY : DRAEGER INC

CUSTOMER PURCHASE ORDER NUMBER : US44302368647

PACKING LIST NUMBER : 21272590

CERTIFICATION DATE : April 26, 2021

ANALYSIS BY : Steven Plutchen  
Quality Representative

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410)228-6400 Fax: (410)228-4251

# ANALYSIS CERTIFICATION

METHOD OF PREPARATION : GRAVIMETRIC / PRESSURE TRANSFILLING

METHOD OF ANALYSIS : IR Breath Alcohol Analyzer

ACCURACY :  $\pm 0.002$  BrAC or  $\pm 2\%$  whichever is greater.

LOT NO. & QTY.	COMP. 1 C <sub>2</sub> H <sub>5</sub> OH	COMP. 2 N <sub>2</sub>	COMP. 3	COMP. 4	COMP. 5	COMP. 6	Exp Date
1346773 (24)	208.4PPM						
	(0.080 BrAC)	BALANCE					07/08/23

## TRACEABILITY

### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited Company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 121088, 121097, 121091, or 121100 dated, 18th January 2019 applies.

WEIGHT SETS USED: Kit #92231, Test #2740564, Kit # 03610, Test # VA-19-1135 T3 Test # VA-19-11350B, T5 Test #VA-19-11350F, VA-19-11350E, VA-19-11350D, IM1966 Test VA-18-11340H

No affecting environmental conditions during analysis.

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

REQUESTED BY : DRAEGER INC

CUSTOMER PURCHASE ORDER NUMBER : UH54302105642

PACKING LIST NUMBER : 16572762

CERTIFICATION DATE : July 8, 2020

ANALYSIS BY : Steve Plutschel  
Quality Representative

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410)228-6400 Fax: (410)228-4251

**CERTIFICATE OF ANALYSIS**  
**EBS - ETHANOL BREATH STANDARD**

DRAEGER INC HOUSTON  
HOUSTON, TX 77085

REF#: 22053560  
DOC#: US44302425104  
CUST. ITEM #: 4401040  
DATE: Jul. 16, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 1523726  
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: Jul. 16, 2024

COMPONENT	PPM	( BrAC )
ETHANOL	416.8	(0.160)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

\* Certification traceability is recognized by NIST through the CIPM MRA.

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.  
Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

**Analytical:**


Analytical Instruments Calibrated Using NMI Traceable Standards.  
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: Jul. 16, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY : 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410)228-6400 Fax: (410)228-4251

**CERTIFICATE OF ANALYSIS**  
**EBS - ETHANOL BREATH STANDARD**

DRAEGER INC HOUSTON  
HOUSTON, TX 77085

REF#: 21766042  
DOC#: US44302404557  
CUST. ITEM #: 4401041  
DATE: Jun. 11, 2021

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 1495468  
ETHANOL IN NITROGEN

PRODUCT EXPIRATION: May. 14, 2024

COMPONENT	PPM	( BrAC )
ETHANOL	781.5	(0.300)
NITROGEN	BAL	

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND50144	260.6

\* Certification traceability is recognized by NIST through the CIPM MRA.

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.  
Calibration test 219908, 219911, 219909, or 219926 dated, 6th January 2021 applies.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.  
Certification Numbers: ND50144-20201218, A679, ND18363-20191203, A650

No affecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

MANUFACTURED DATE: May. 14, 2021

CALGAZ CYLINDER SIZE: 6D

APPROVED BY :



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410)228-6400 Fax: (410)228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 1109411181

Date: April 08, 2022

**NJSP DEPT of LAW and PUBLIC SAFETY**

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402396000

ETHANOL IN NITROGEN

Product Expiration: March 21, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	260,5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	261.0	(0.100)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: March 21, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

**DRAEGER MEDICAL SYSTEMS INC.;**

Sales order: 1109388535

Date: April 26, 2022

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402410761

ETHANOL IN NITROGEN

Product Expiration: April 14, 2025

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL.	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	263.0	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38434	260.4

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

#### TRACEABILITY

##### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Calibration test 283190, 283189, 283188, or 283192 dated 6th January 2022 applies

##### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: ND38434-20211028, A679, A650, ND38462-20211027, ND18363-20211104, ND50144-20201218


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 14, 2022

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251





# Dräger

## Alcotest 9510

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

6/14/2022

ARMH-0287

Draeger, Inc. GR MB

DEPARTMENT OF  
**Law and Public Safety**  
*This is to certify that*

**Kevin W. Alcott**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

*[Signature]*

COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*

ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/18)

DEPARTMENT OF  
**Law and Public Safety**  
*This is to certify that*

**Kevin W. Alcott**

**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 9510

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 8th DAY OF June

TWO THOUSAND AND Twenty One

*[Signature]*

COLONEL  
 NEW JERSEY STATE POLICE

*[Signature]*

ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/18)